

SPECIFICATION SHEET



ORGANIC POLLUTION MONITOR UV METER

OPM-1610

Organic Pollution Monitor UV Meter OPM-1610 is an ultraviolet absorbance spectrophotometer that has been commercialized based on our over 30 years of experience and results. This instrument is used to determine the degree of organic pollution in wastewater discharged from factories and business sites from the absorbance of ultraviolet rays. The calculated values are correlated with CODMn and are used to calculate the pollutant load associated with the total water quality control. Make sure that good correlation is obtained beforehand.



Feature

○Achieved miniaturization

The immersion type detector, which has been well received by conventional machines, has been downsized, enabling simple installation. It can also be used as a water sampling system by using a receiving tank.

○Adopt a new type of optical system

- Stable measurement by feedback control of light intensity has been realized
- Use of power-saving lamps and other factors allowed elimination of a heater to stabilize the light intensity of the lamp, dramatic reduction of power consumption reduced (by approximately 80% compared to our previous model). The immersion type also eliminates the need for sampling pumps, enabling further power savings.

○Equipped with anti-corrosion zinc as standard

It is resistant to corrosion and is also suitable for measurement in poor environments.

Transmission output range : The upper limit is 0.5 to 2.5 in 0.1 increments.

The lower limit is fixed to "0".

The measured value can also be displayed in

10mm cell length conversion absorbance.

0 to 1.0Abs for 25mm cells.

0 to 2.5Abs for 10mm cells

0 to 4.17Abs are displayed for 6mm cells

Measurement cell : Immersion Parallel Cell

(Select from 6mm, 10mm, 2mm)

Cell cleaning method : Automatic cleaning with a wiper

Wash cycle: 1 to 9999min (60 for initial setting)

Numbers of washes: 0 to 99 (2 for initial setting)

Wait time after washing: 0 to 999 sec (10 for initial setting)

Sample water condition : Sample water temperature: 0 to 45°C (do not freeze)

Flow rate (immersion type): 0.75m/sec or less

(Note on installation on pages 7 and 9)

Flow rate (sampling type) 3 to 6L/min

Detector max water depth : 6m

Calibration method : Zero calibration: with pure water

Span calibration: with potassium hydrogen phthalate solution

(The calibration container is a standard accessory.)

Indicatable items : UV-VIS/UV/VIS/COD conversion value/turbidity conversion value/SS concentration/sample water temperature

Standard specification

Product name : Organic Pollution Monitor UV Meter
Model : OPM-1610
Measurement target : Organic pollutants in wastewater from factories, workplaces, etc.
Measurement method : 2-Wavelength Absorbance Spectrometry (ultraviolet light (UV); 254nm, visible light (VIS);660nm).
Measurement range : UV absorbance; 0 to 2.5Abs

Transmission output : DC 4 to 20mA load resistance 600Ω or less insulated type
Any 3 types from UV-VIS/UV/VIS/COD conversion value/Turbidity conversion value/SS concentration conversion value/Sample water temperature can be selected and output simultaneously (non-insulated between transmission outputs) COD conversion value/turbidity conversion value/SS concentration conversion value is the value of the primary formula conversion from absorbance.

Contact output signal : Alarm signal a (NO) contact output (Any 3 points can be selected and used for contact outputs 1 to 3 from the following 9 items)
Maintenance in progress
Cleaning in progress
Bulk alarm*
Measured value upper limit alarm
Lamp error
No sample water
Leakage alarm
Wiper drive motor failure
Sample water temperature error
*PV high limit alarm, lamp failure, no sample water, water leakage alarm, wiper drive motor error, and sample water temperature abnormalities are included in the alarms
Power-off signal c (NO/NC) Fixed to contact output 4
Contact Capacitance DC 30V 0.1A or less
AC 125V 0.1A or less (resistive load)

Contact input signal : Clean start signal... by external program for cleaning control
Non-voltage contact input
ON-resistance 50 Ω or less, short-circuit current max. 5 mA, open-circuit voltage DC 24V, make time 0.1 sec. or more

Digital output (Optional) : Communication output RS-485 or USB memory for data recording
●Digital communication output
Interface RS-485
●USB memory (data in CSV format)
Memory contents: year, month, day, hour, minute, UV value, VIS value, COD-equivalent, turbidity-equivalent, SS-concentration-equivalent, and water temperature values
Sampling period: can be arbitrarily set from 1 to 999 min
Storage period: approximately 5 years of data stored at 1 minute sampling period.
When free space is exhausted, data cannot be written. Periodically delete old data.

Power source : AC 100 to 240V±10% 50/60Hz
Power consumption : Av. approx 10VA, Max approx. 20VA
Mounting method : immersion type, winding type, suspending type, water sampling type
Main materials : Transmitter : aluminum die-casting
Detector: Main unit...SUS316, PP, zinc, silicone rubber
Cell...Sapphire glass
Wiper...FPM or SUS304

Coating color : Transmitter: metallic silver

Protective construction : Transmitter: IP65

Transmitter wiring port : Cable gland 6 points (Diameter for φ6 to φ12)
(1 among them is for detector cable)
Cable ground can be removed and the cable can be connected (G1/2×6)

Dedicated cable : 1 cable from detector to transmitter
Standard length: water sampling formula 3m
Length is specified for immersion type, winding type, and suspending type up to 30m (optional)

External dimension (refer to the dimension drawing) : Transmitter:
Approx 181(W)×95(D)×180(H)mm
Detector:
Approx 148(W)×112(D)×437(H)mm
(not including connecting cable)

The immersion type (H) varies depending on the specification

Weight : Transmitter: Approx. 2.0kg
Detector: Approx 5.9 kg (Not including cable weight)

Installation condition : Outdoor installation available
Ambient temperature: -5 to 50°C
Ambient humidity (transmitter):
95% RH or less

Free from vibration, impact and corrosive gases. The location where the detector is installed should be such that the sample water is substituted, which can be representative of the value of the sample water.

Related equipment : Load Calculator: When calculating pollution load, CALD-2030 loading calculator is recommended.

Features


UV absorbance linearity : Within $\pm 2\%$ FS (by calibration solution)
 UV absorbance repeatability : Within $\pm 2\%$ FS (by calibration solution)
 UV absorbance zero drift : Within $\pm 2\%$ FS/week
 UV absorbance span drift : Within $\pm 2\%$ FS/week
 (FSs have 2.5Abs of UV-absorbance)
 Responsiveness : 90% response within 30seconds

Estimated value of COD conversion output by cell length

Cell length	COD value (mg/L)
25mm	0 to 50
10mm	50 to 100
6mm	100 to 500

Immersion type parallel cell
 (select from 6mm, 10mm, or 25mm)

Principle of operation

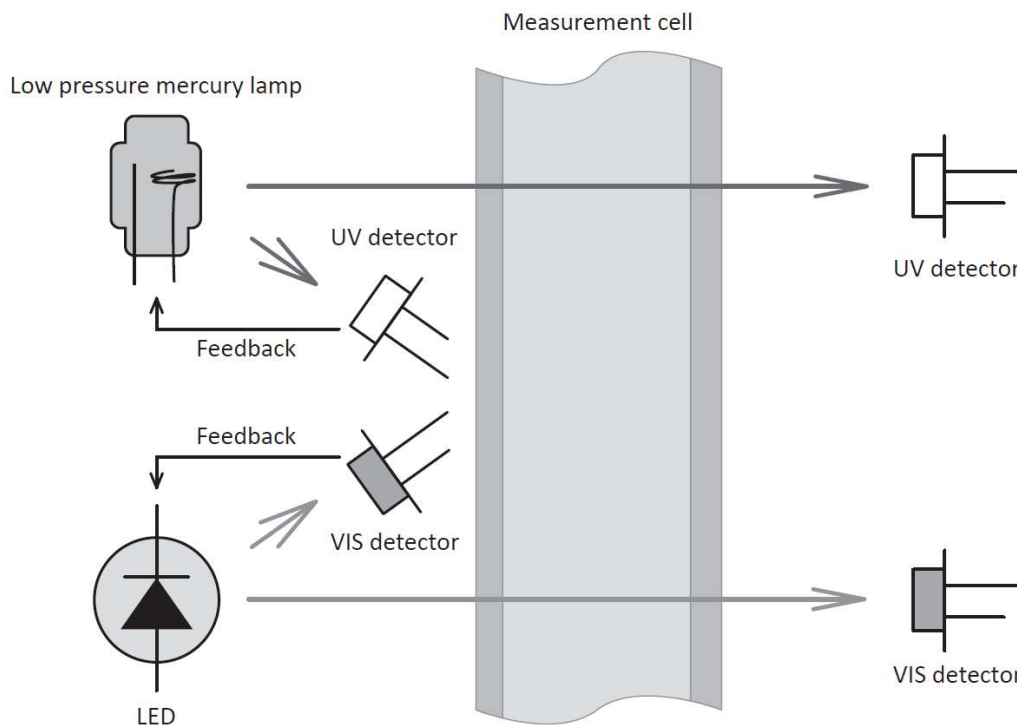


The measurement is performed using a two wavelength light source that stabilizes the two light quantities of UV (ultraviolet light) and VIS (visible light).

UV measurement uses the bright line of an ozoneless low-pressure mercury lamp at 254nm. VIS measurement is performed by irradiating an LED at 660nm with a pulse light to measure turbidity.

Conversion to COD value may be used by determining the correlation between the value obtained by the absorbance AUV of UV and COD manual analysis value, or by determining the correlation between the value $AUV - \alpha \times AVIS$ obtained by excluding the absorbance AVIS of VIS due to the effect of turbidity and the COD manual analysis value.

α =correction factor (can be arbitrarily set).


Terminal connection diagram

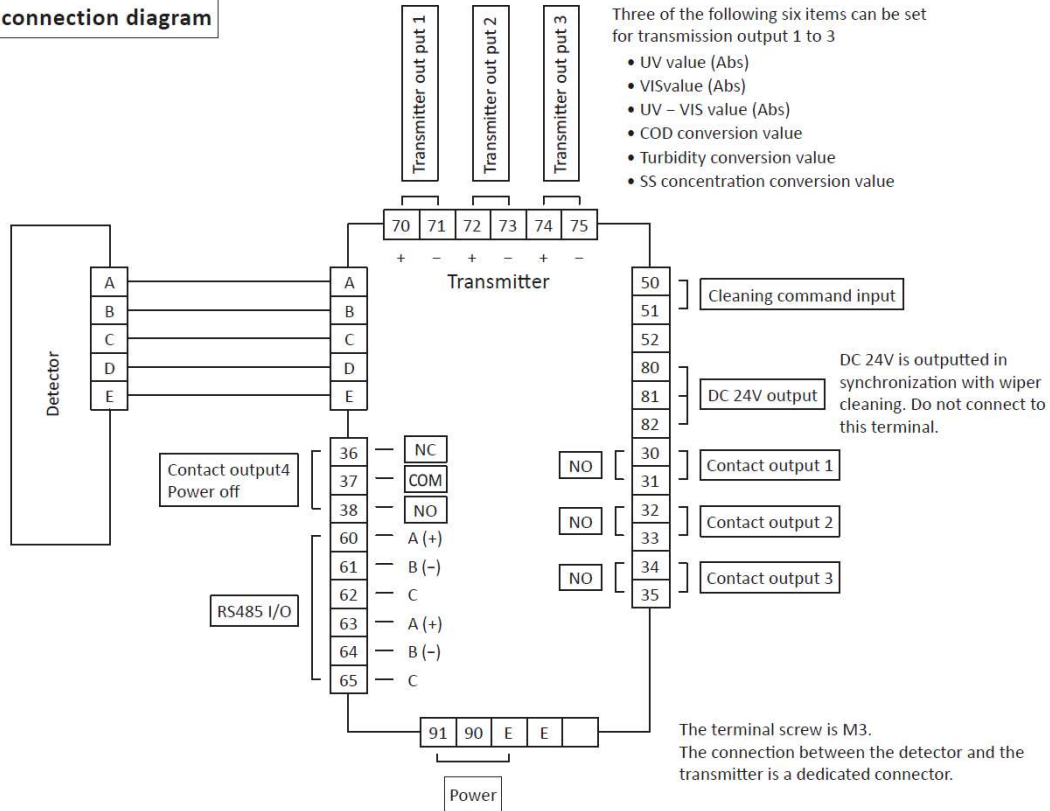


Dimensions

Unit : mm

● Pole mounting

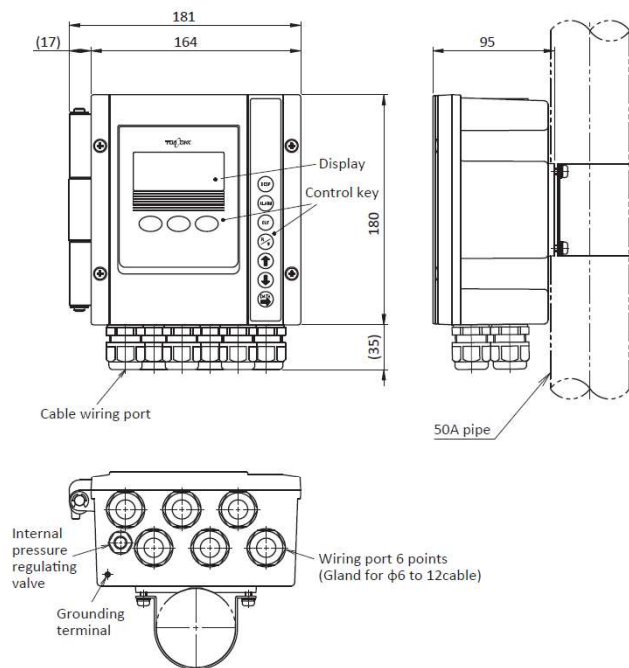

● Installed on a wall or rack

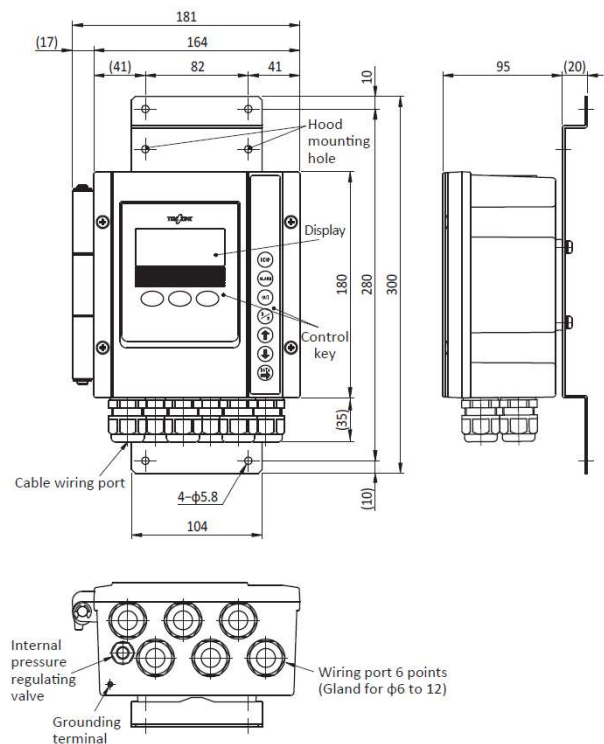

● Hood (option)

It is recommended for installation under direct sunlight outdoors.

Material : SUS304


Mounting methods : 50 A pipe or wall mounted

Code No. : 7049930K


Dimensions

Unit : mm


● Detector for immersion type

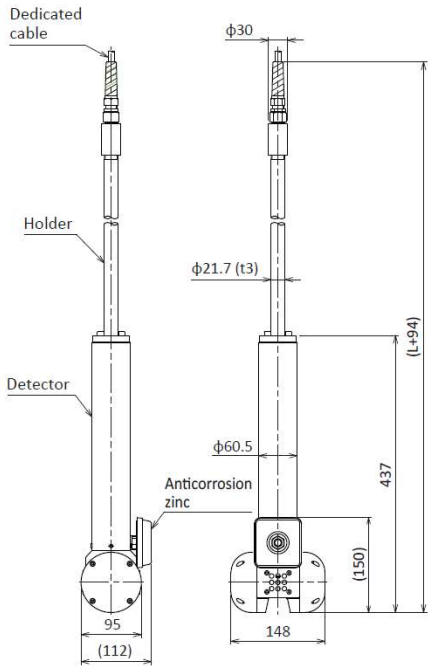


● Detector for winding type
[For one guide pipe]

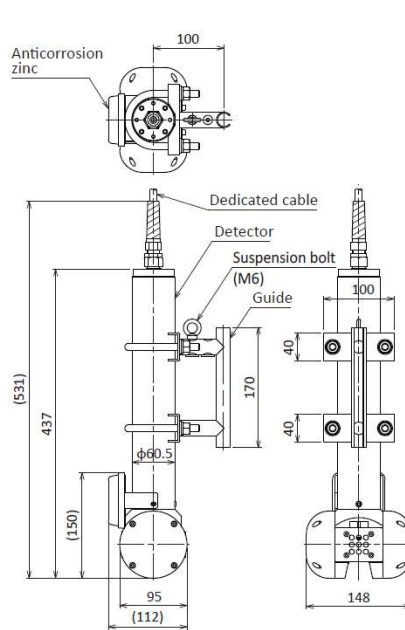


[For two guide pipes]

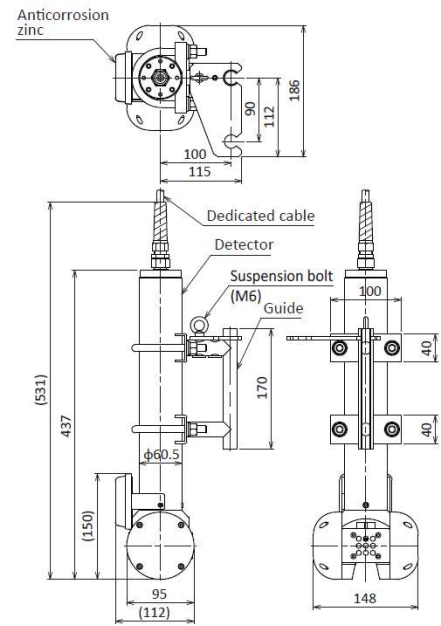

● Detector for Suspending type

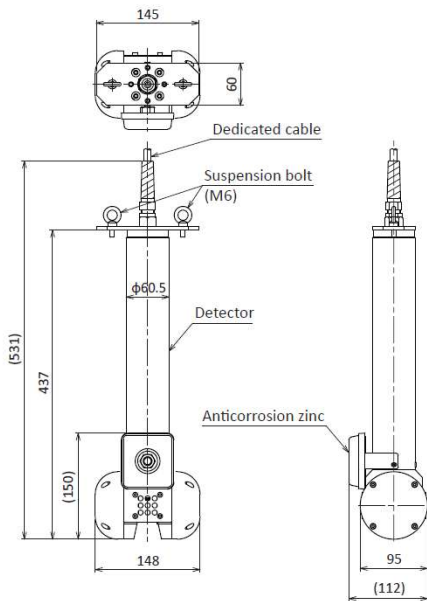

● Detector for water sampling type

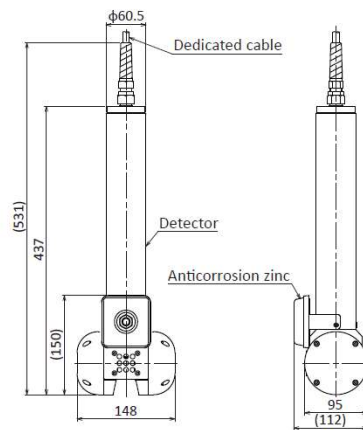


Installation



Unit : mm

● Immersion type

1. Platform installation dimensions Maintenance space and foundation bolt position

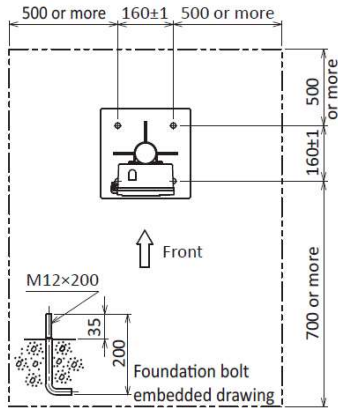

2. Outer dimensions of frame

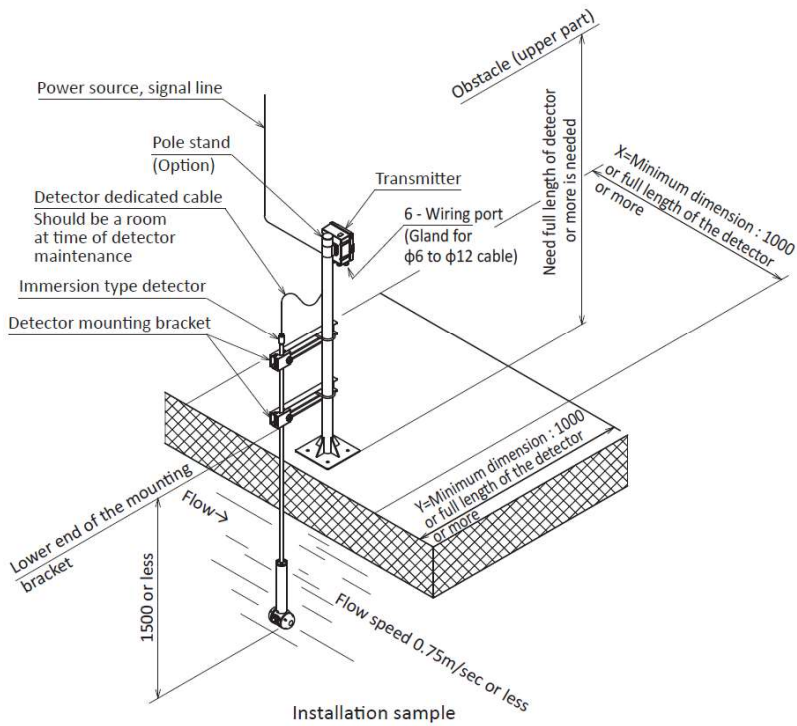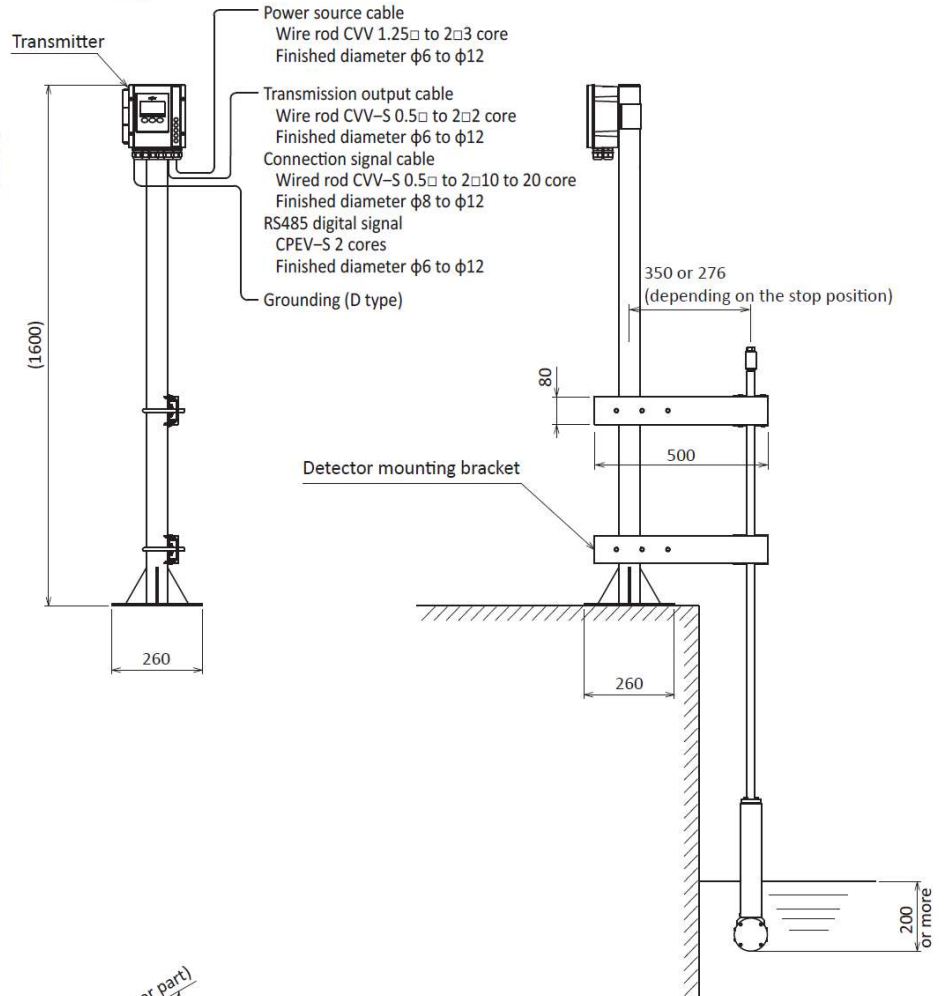

(Notes)


1. Install the detector so that the pulling-up work during maintenance can be performed easily and safely. Also consider the force acting on the lower end of the detector due to the weight and flow velocity of the detector, and firmly mount the detector.
2. Secure a space of at least the full length of the detector so that the detector can be placed in the X or Y direction of the maintenance space. (Refer to the drawing)
3. The minimum liquid level depth of the detector should be 200mm or more.
4. When routing the dedicated cable (accessory) between the detector and the transmitter, pull up the detector so that maintenance and inspection can be performed. Also, keep the dedicated cable away from noise sources such as power lines.
5. Grounding should be Class D grounding and separate from power grounding.
6. Be sure to install an earth leakage breaker on the power supply line.
7. The shape of the pole stand and detector mounting bracket differs depending on the specifications. Refer to the delivery specifications.

Installation

Unit : mm

● Winding / Suspending type


1. Other dimensions of frame

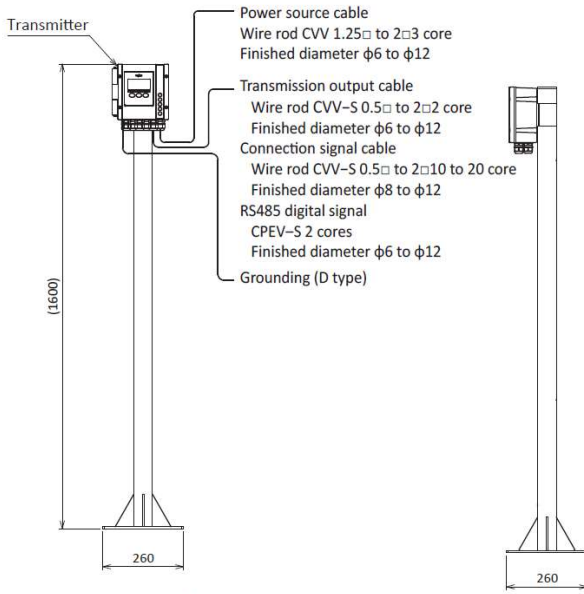


External diameter of winding machine
(Example : For 2m guide pipe
Note) If the take-up winch is made of stainless steel, the handle and fixed position are symmetrical.

● Winding machine

(For one guide pipe)

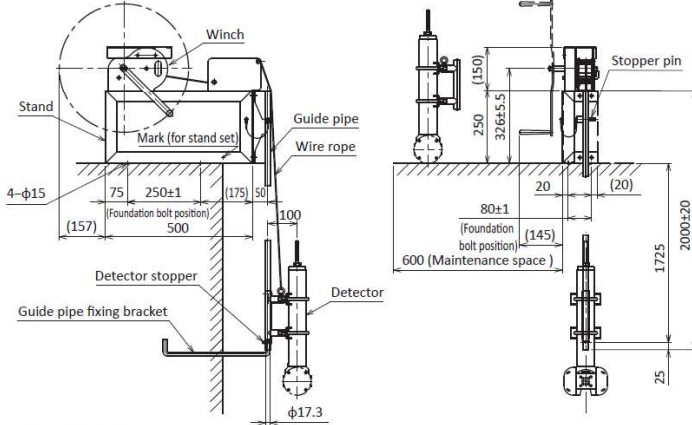


(For two guide pipes)

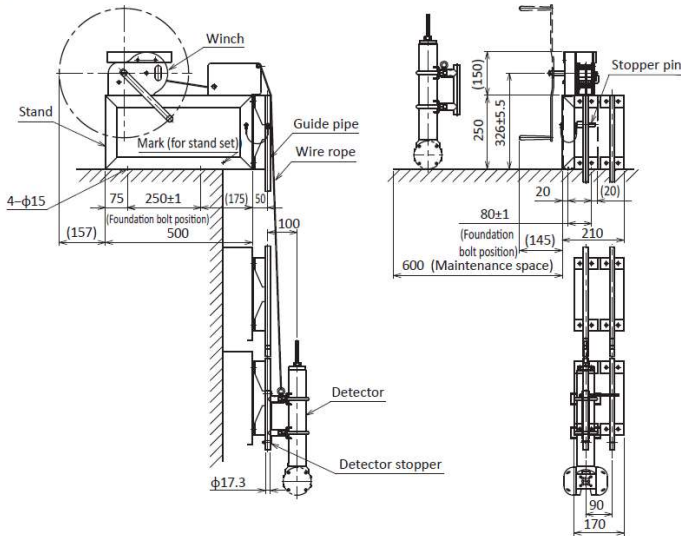


2. Platform installation dimensions

Maintenance space and foundation bolt position

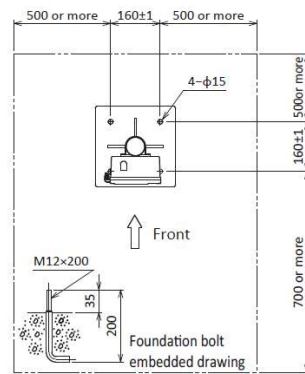


3. Winding device installation

Foundation bolt position

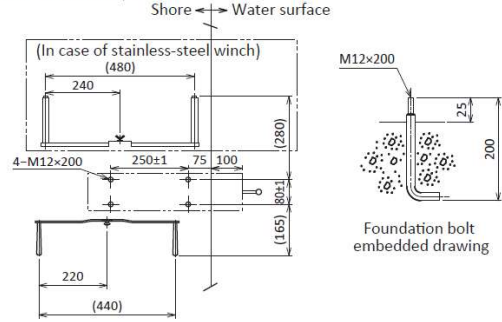


Fixing of guide pipe (1 P)

Prepare a fixing bracket as shown in the figure below and fix onto a sea wall

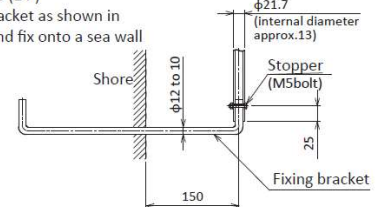





● Suspending type

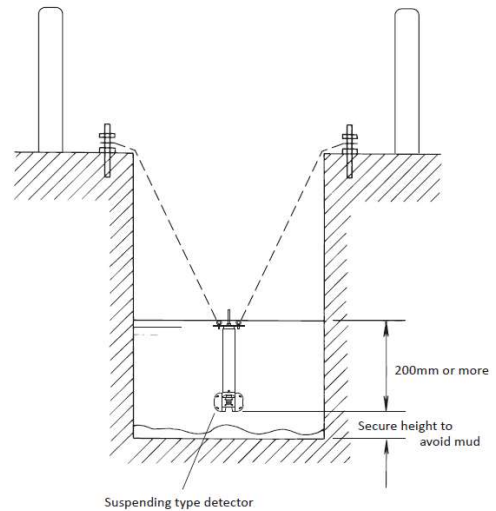




Installation

Unit : mm

● Water sample type (Pole stand mounting)

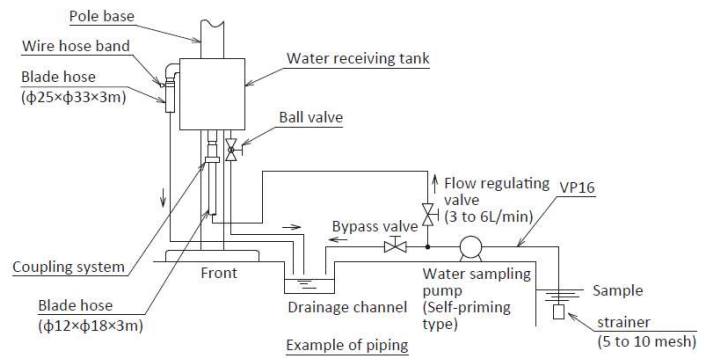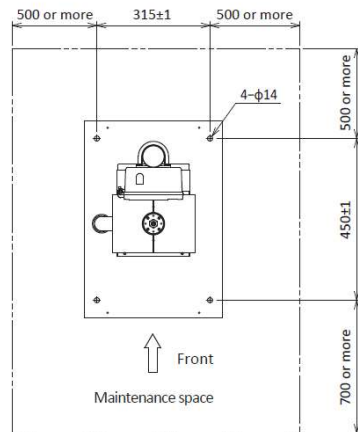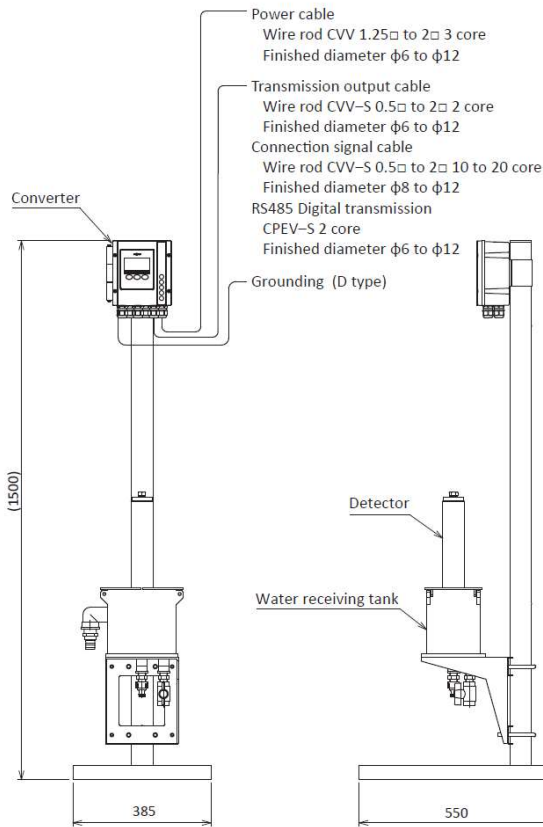

● Water sampling type (aluminum frame mounting)

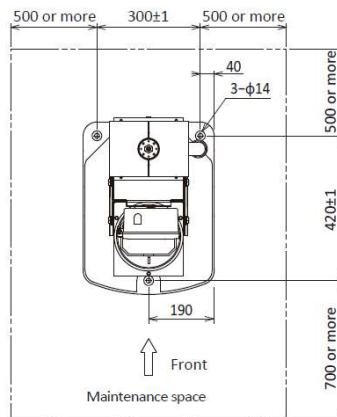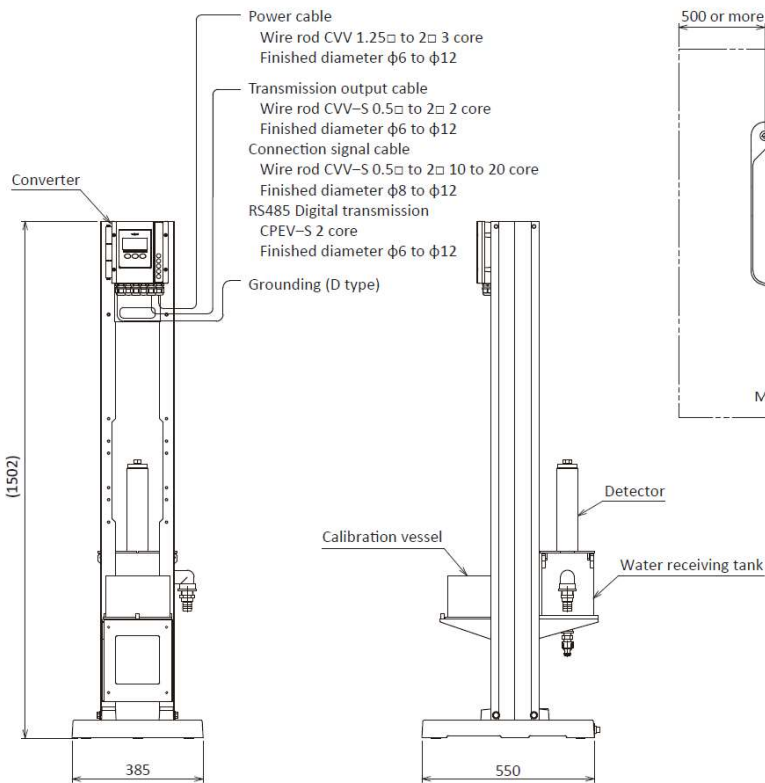



DKK-TOA CORPORATION

Overseas Sales Division:
DKK-TOA Corporation
29-10, 1-Chome, Takadanobaba, Shinjuku-ku,
Tokyo 169-8648 Japan
Tel : +81-3-3202-0225 Fax : +81-3-3202-5685
E-mail : intsales@dkktoa.com



Please read the operation manual carefully
before using products.

<https://www.toadkk.com/english/>

Information and specifications are subject to change without notice.